


SQC

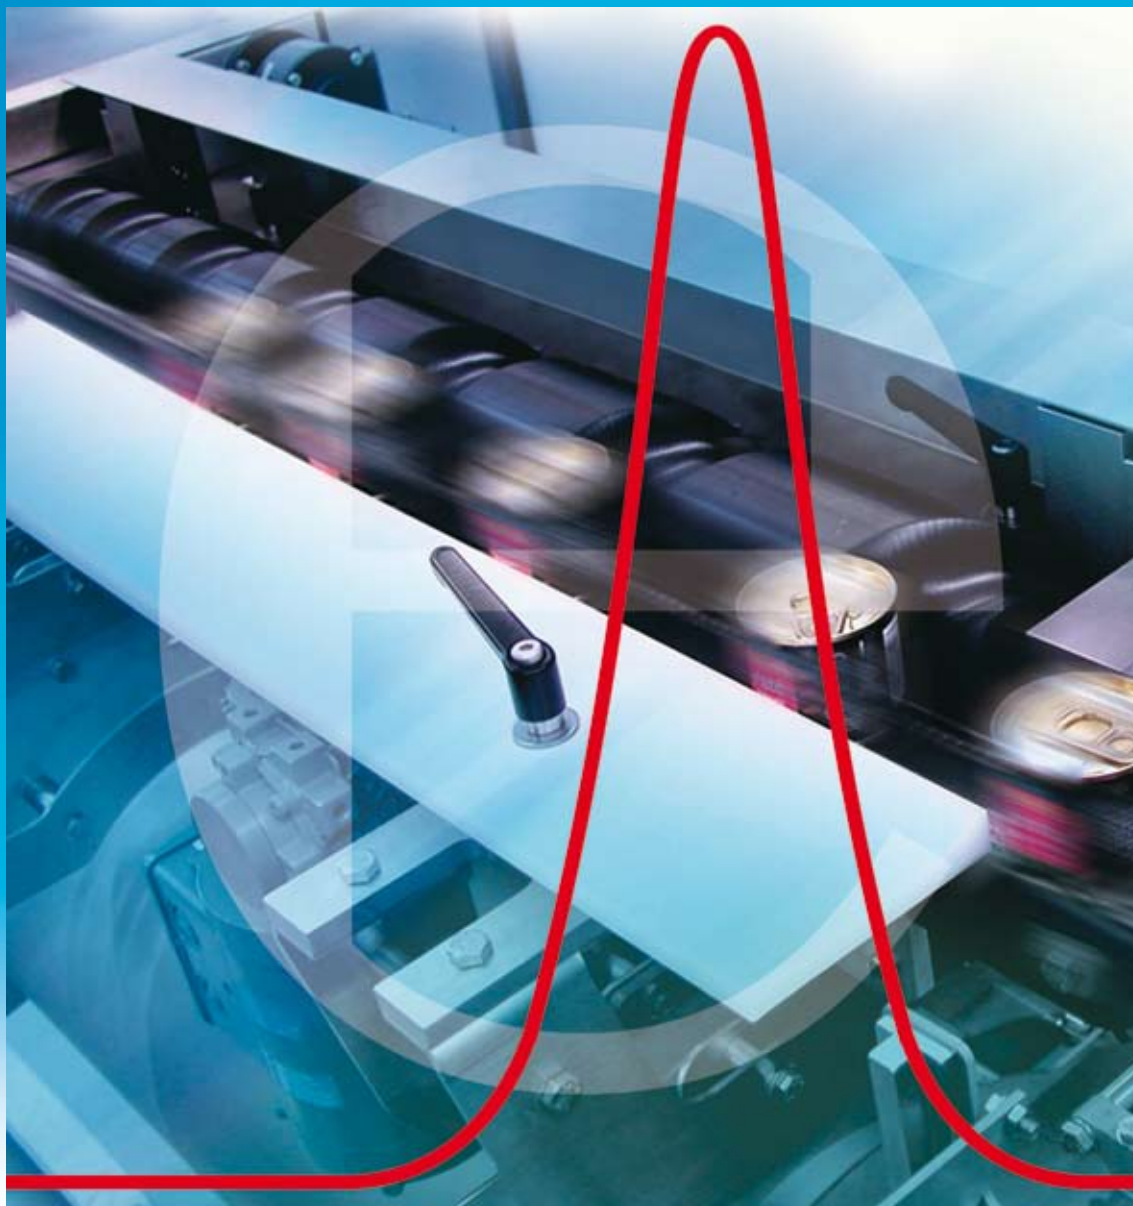


FreeWeigh.Net®

New dimensions in process control

METTLER TOLEDO

Just a few steps to documented quality


FreeWeigh.Net® helps you get results faster. Just five simple and clear steps are required from the specification of your product right up to detailed results.

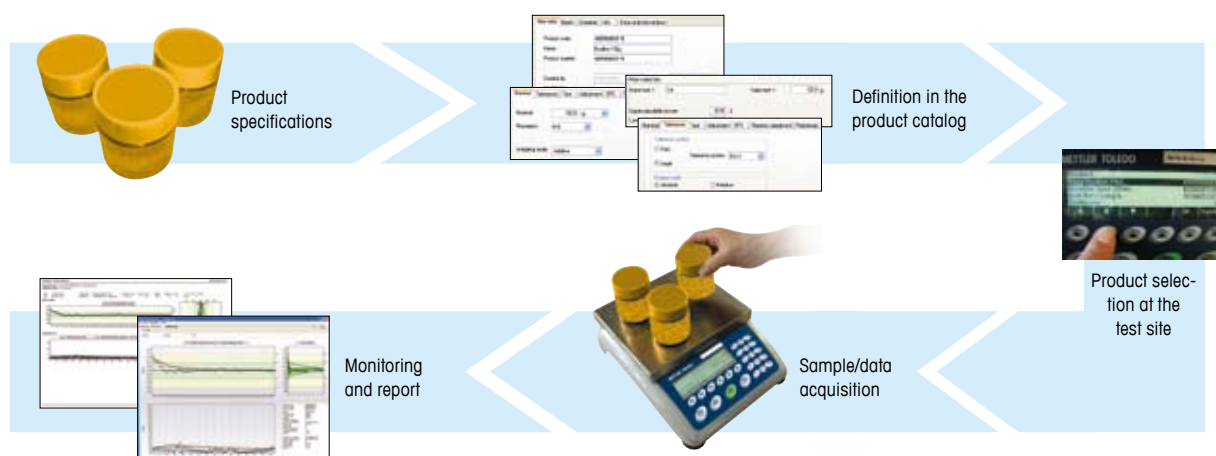

Comprehensive quality control with FreeWeigh.Net®

Alongside checking the fill quantity, FreeWeigh.Net® also allows you to record, monitor and document a range of quality parameters – whether additional measured values, such as the tightness of a package, torque of a bottle cap or friability of a tablet. If the measuring device used has a data interface, the re-recorded values can also be automatically transferred to FreeWeigh.Net®.

Attributive quality parameters, such as expiry date, batch number, color or taste can be recorded simply and quickly using the FreeWeigh.Net® attribute module and then visualized, for example in a Pareto chart.

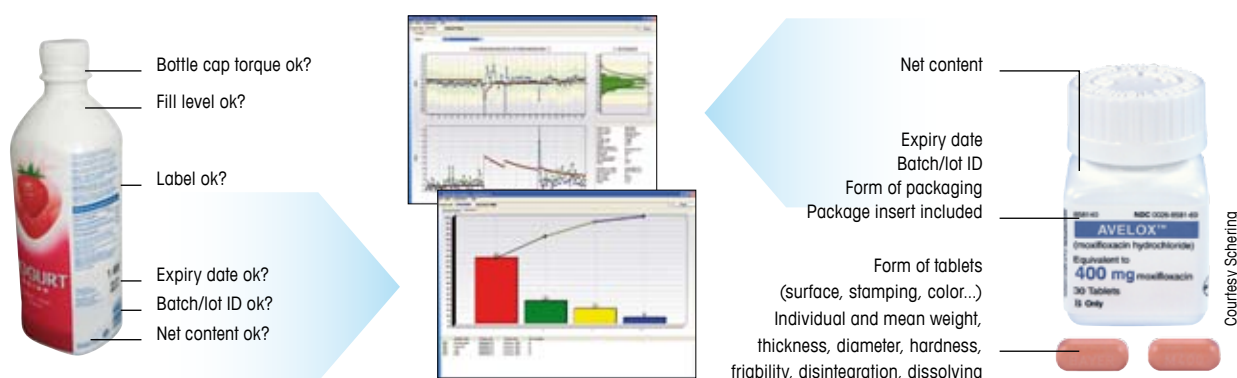

Maximize profitability

And at the same time respect legal requirements



Your filling process is always under control thanks to online monitoring from FreeWeigh.Net®.

If you discover a deviation during the manufacturing process, you can immediately intervene to make a correction and achieve the optimum fill quantity without violating the legally required minimum fill quantities.

Once a production batch has been completed, you know exactly which mean value, variation and standard

deviation it has without having to wait for handwritten record sheets to be evaluated.


This results in optimized production profitability, while compliance with standards is documented in black and white.

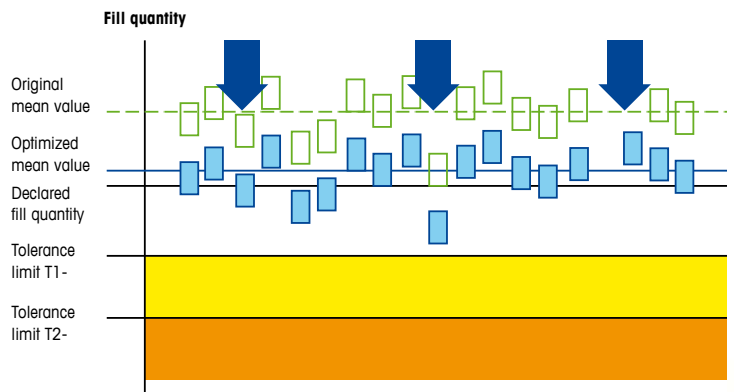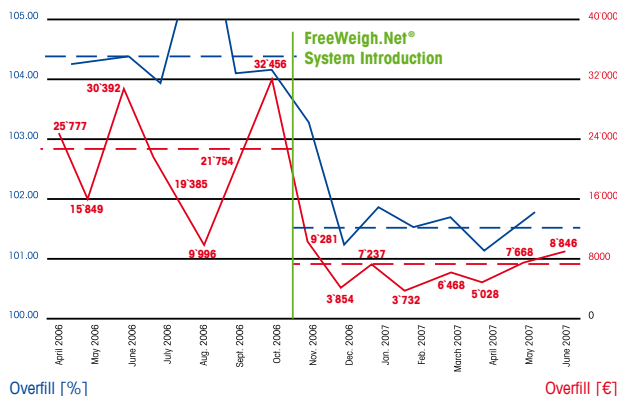

Meets the strict demands of the pharmaceutical industry

As well as complying with GMP/GAMP regulations, the computer system validation (CSV) defines, assigns and guarantees the reliability and consistency required in the process performance.

This not only includes the FreeWeigh.Net® system, but also the fully traceable development processes at METTLER TOLEDO, which make FreeWeigh.Net® an ideal quality control system for the pharmaceutical industry.

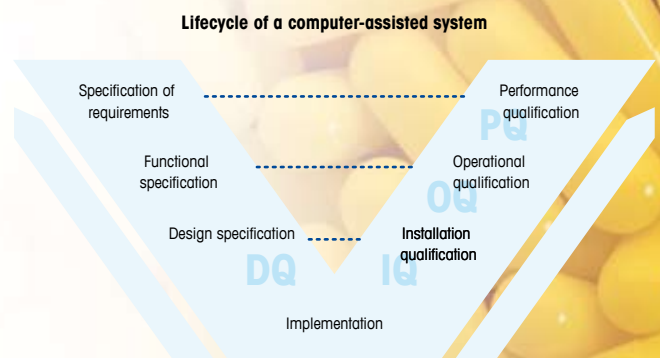

FreeWeigh.Net®

The quality of your products is the most important factor



The central product catalog contains all test item definitions



Space-saving solutions with remote balances



Job preparation with central database




IT administration and maintenance



MS SQL database




Automated checkweighing and metal detection

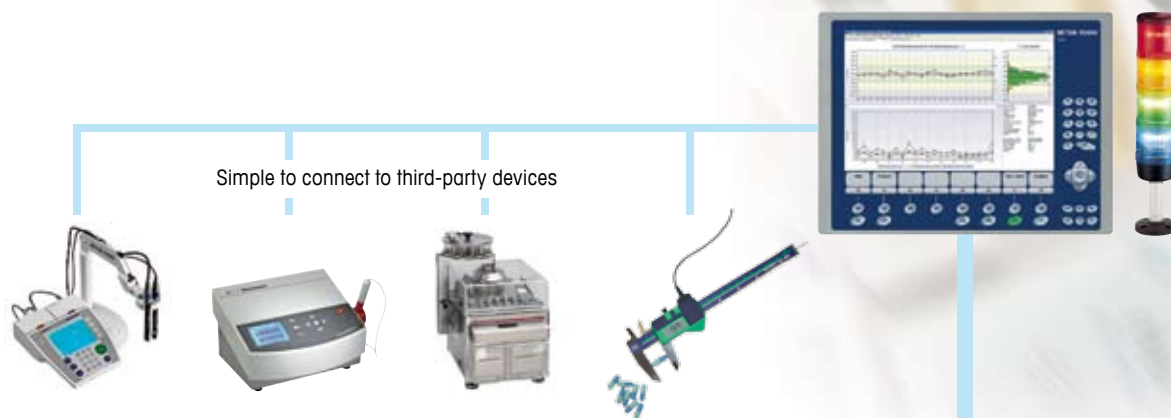

Monitoring & documentation
in the office



Execution and data acquisition is
quick and easy to understand

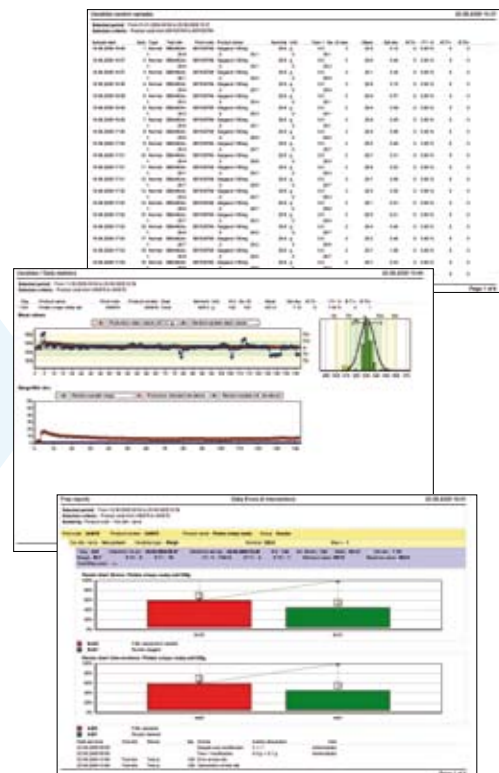

Devices in the FreeWeigh.Net® quality control system are connected to the in-house computer network. All the data recorded here is stored in the central data server. The immediately updated statistics are transmitted as a confirmation to the test sites and automatically displayed on the monitoring systems.


The modular system architecture allows quick and simple adjustments to new operating conditions.

A wide range of standard devices and specialized instruments are available for operation with the FreeWeigh.Net® system. The performance and design of this equipment allows it to be used in many different applications and ambient conditions. Additional devices can be operated using the configurable third-party device integration module.


FreeWeigh.Net® – Keeping your quality fully under control




The FreeWeigh.Net® testplace module is the PC-based workstation which controls connected devices.

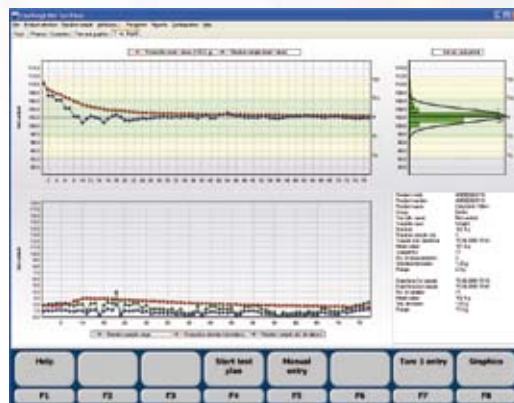

Online feedback on the FreeWeigh.Net® testplace module. Updated statistics are immediately available.

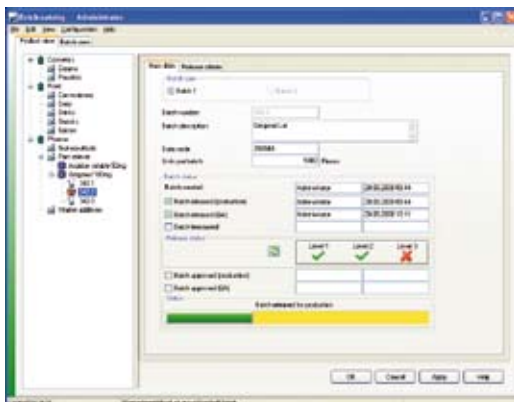

The FreeWeigh.Net® batch catalog manages up to two batches running in parallel per product.

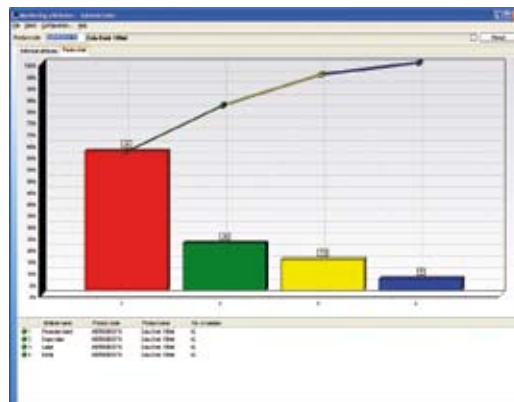

Attributive product defects can also be visualized by FreeWeigh.Net® in the Pareto chart.

Criteria	Level 1	Level 2	Level 3
Batch 1: 340.2	✓	✓	✗
Product: 980743574 / Equipment 18195			
From: 20.08.2008 08:13 To: 20.08.2008 18:25			
Summary: Product 1: 1497			
The mean value is greater than or equal to the nominal value	Value: 50.8 Limit: 50.8	Value: 50.8 Limit: 50.8	Value: 50.8 Limit: 50.8
Max destructive test: mean 1 = Nominal: 47 * s	Value: 50.8 Limit: 50.8	Value: 50.8 Limit: 50.8	Value: 50.8 Limit: 50.8
Minimum number of sample errors	Value: 27 Limit: 27	Value: 27 Limit: 27	Value: 27 Limit: 27
Minimum number of individual values	Value: 15 Limit: 15	Value: 15 Limit: 15	Value: 15 Limit: 15
The number of T2- violations is smaller than or equal to	Value: 1 Limit: 1	Value: 1 Limit: 1	Value: 1 Limit: 1
The number of T2+ violations is smaller than or equal to	Value: 1 Limit: 1	Value: 1 Limit: 1	Value: 1 Limit: 1
The number of T2- violations is smaller than or equal to	Value: 1 Limit: 1	Value: 1 Limit: 1	Value: 1 Limit: 1
The number of T2+ violations is smaller than or equal to (Phases 1/2)	Value: 1 Limit: 1	Value: 1 Limit: 1	Value: 1 Limit: 1
The number of T2+ violations is smaller than or equal to (Phases 1/2)	Value: 1 Limit: 1	Value: 1 Limit: 1	Value: 1 Limit: 1
Max destructive test: mean 1 = Nominal: 47 * s	Value: 50.8 Limit: 50.8	Value: 50.8 Limit: 50.8	Value: 50.8 Limit: 50.8

For each batch, individual criteria for release can be defined. FreeWeigh.Net® monitors this to ensure that the criteria are met.

Sample Failed
Please complete your entries and contact your shift supervisor

Product name: Potato crisps ready salt 530g
Product code: 345678
Nominal: 529.0 g
Mean value: 513.9 g
Minimum value: 513.9 g
No. of T2- violations: 0
Mean value: 513.9 g
<T1-: 1
<T2-: 0

Net content

Error: Em01 - Nozzle clogged
Intervention: In01 - Nozzle cleaned

OK Cancel

The optional module «Errors & Interventions» enables you to enter the reasons for errors and the action taken in production.

FreeWeigh.Net® – The full-scope solution for your quality control



What you require

- Minimization of overfilling and reduction in material costs
- Quick process rectification options based on online data analysis
- Compliance with net content legislation – fast and guaranteed availability of historical data as documented evidence for a comprehensive Q analysis
- Compliance with the FDA and other regulations with regard to audit trail and process control, such as 21 CFR part 11
- Simplification and rationalization of quality control processes

What you stand to gain

- Better utilization of material batches
- Standardized operational procedures and processes
- Accelerated data acquisition and elimination of incorrect entries
- Standardized and automatic reporting
- Faster return on investment
- Improved filling accuracy and maximized profitability

What we promise to provide


- A modern and continuously updated system for comprehensive quality control
- Linear extendibility and flexible adaption to changing conditions
- Central data storage with maximum availability
- Ideal interaction between software, hardware and peripherals
- Maximum investment protection through long-term product maintenance and proven upgrade strategies
- Intuitive operation and simple handling
- Space-saving input devices and measuring instruments
- Minimum training requirements and maximum avoidance of operator errors
- Clear, easy to interpret results, from which procedures can be quickly and easily derived



Professional services

METTLER TOLEDO offers you a wide range of professional services that ensure smooth project processing and guarantee you optimum solutions:

- Comprehensive validation documentation (CSV Pac) in two volumes for supplier audits and IQ, OQ and PQ
- Support in project management and coordination through experienced project engineers
- Validation support through trained specialists
- Database and ERP integration

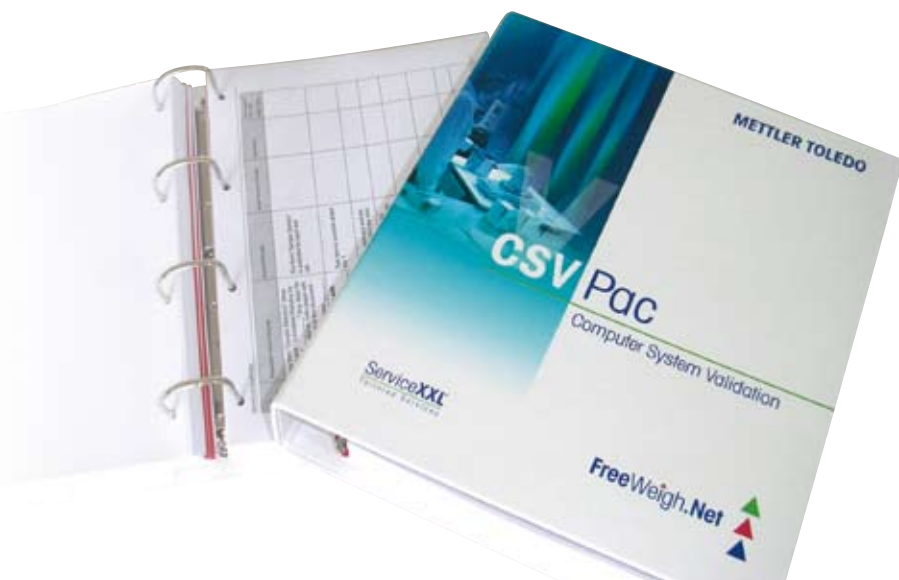

www.mt.com

For more information

Mettler-Toledo AG
CH-8606 Greifensee
Tel. +41-44-944 2211
Fax +41-44-944 3060

Subject to technical changes
© 09/2008 Mettler-Toledo AG
Printed in Switzerland
MTSI 21900891

nefton
Ζύγιση
Σήμανση
Συμμόρφωση

Νεφτών Τεχνολογίες ABEE
Γέρακα 113, Τ.Θ. 67934
15344 Γέρακας
Τηλ: 210 6654544
Fax: 210 6654545
marketing@nefton.gr
www.nefton.gr